



US007972869B2

(12) **United States Patent**  
**Quine et al.**

(10) **Patent No.:** **US 7,972,869 B2**

(45) **Date of Patent:** **Jul. 5, 2011**

(54) **METHOD AND DEVICE FOR COLLECTING AND TRANSFERRING BIOHAZARD SAMPLES**

(58) **Field of Classification Search** ..... 422/50, 422/58, 68.1, 99, 100, 83, 88; 436/177  
See application file for complete search history.

(75) Inventors: **Douglas B. Quine**, Bethel, CT (US);  
**Ashwani Sharma**, Lincoln, ME (US);  
**John E. Massucci**, Eastchester, NY (US);  
**Candace Lee Summers**, Front Royal, VA (US)

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,463,815 B1 \* 10/2002 Tallentire et al. .... 73/863.23  
2004/0045342 A1 \* 3/2004 Jones et al. .... 73/37  
\* cited by examiner

(73) Assignee: **Pitney Bowes Inc.**, Stamford, CT (US)

*Primary Examiner* — Sam P Siefke

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(74) *Attorney, Agent, or Firm* — George M. Macdonald; Charles R. Malandra, Jr.

(21) Appl. No.: **12/371,905**

(57) **ABSTRACT**

(22) Filed: **Feb. 16, 2009**

A method and system for collecting airborne particles and hydrating the collected particles for analysis. The airborne particles, which may be biological contaminants, are collected from a container containing one or more mailpieces. In the collection stage, a dry filter collection assembly is connected to the container and air is drawn out of the container through a dry filter. A hydration solution is then injected into the collection assembly to hydrate the collected particles. Part of the hydration solution containing the collected particles is caused to move out of the collection assembly to a test cartridge for further testing.

(65) **Prior Publication Data**

US 2009/0229384 A1 Sep. 17, 2009


**Related U.S. Application Data**

(63) Continuation-in-part of application No. 10/741,264, filed on Dec. 19, 2003, now Pat. No. 7,491,548.

(51) **Int. Cl.**  
**G01N 33/00** (2006.01)

(52) **U.S. Cl.** ..... **436/177; 422/83**

**20 Claims, 11 Drawing Sheets**

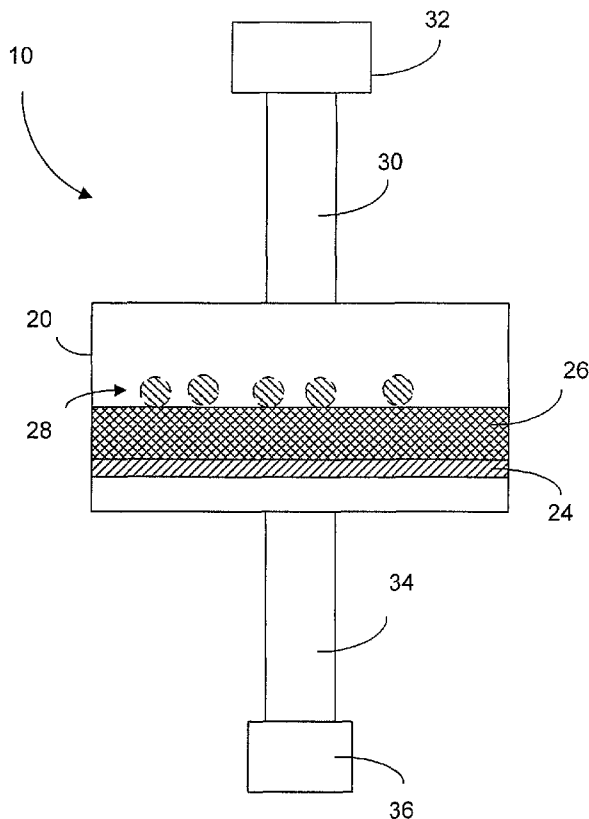

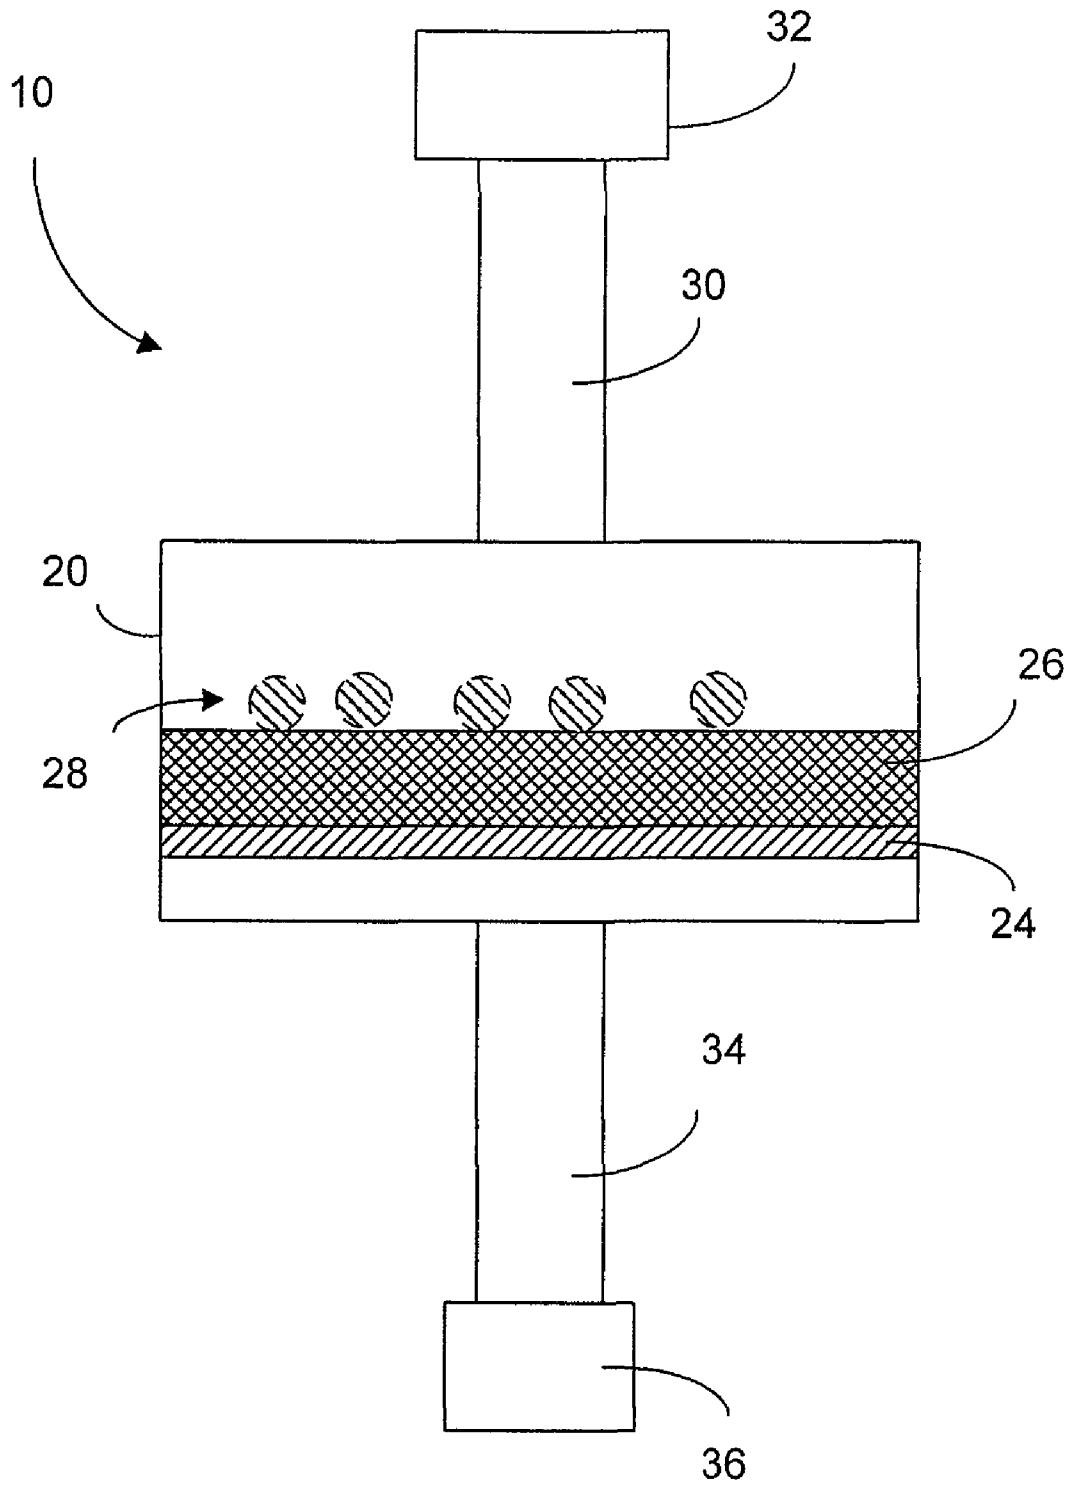


FIG. 1

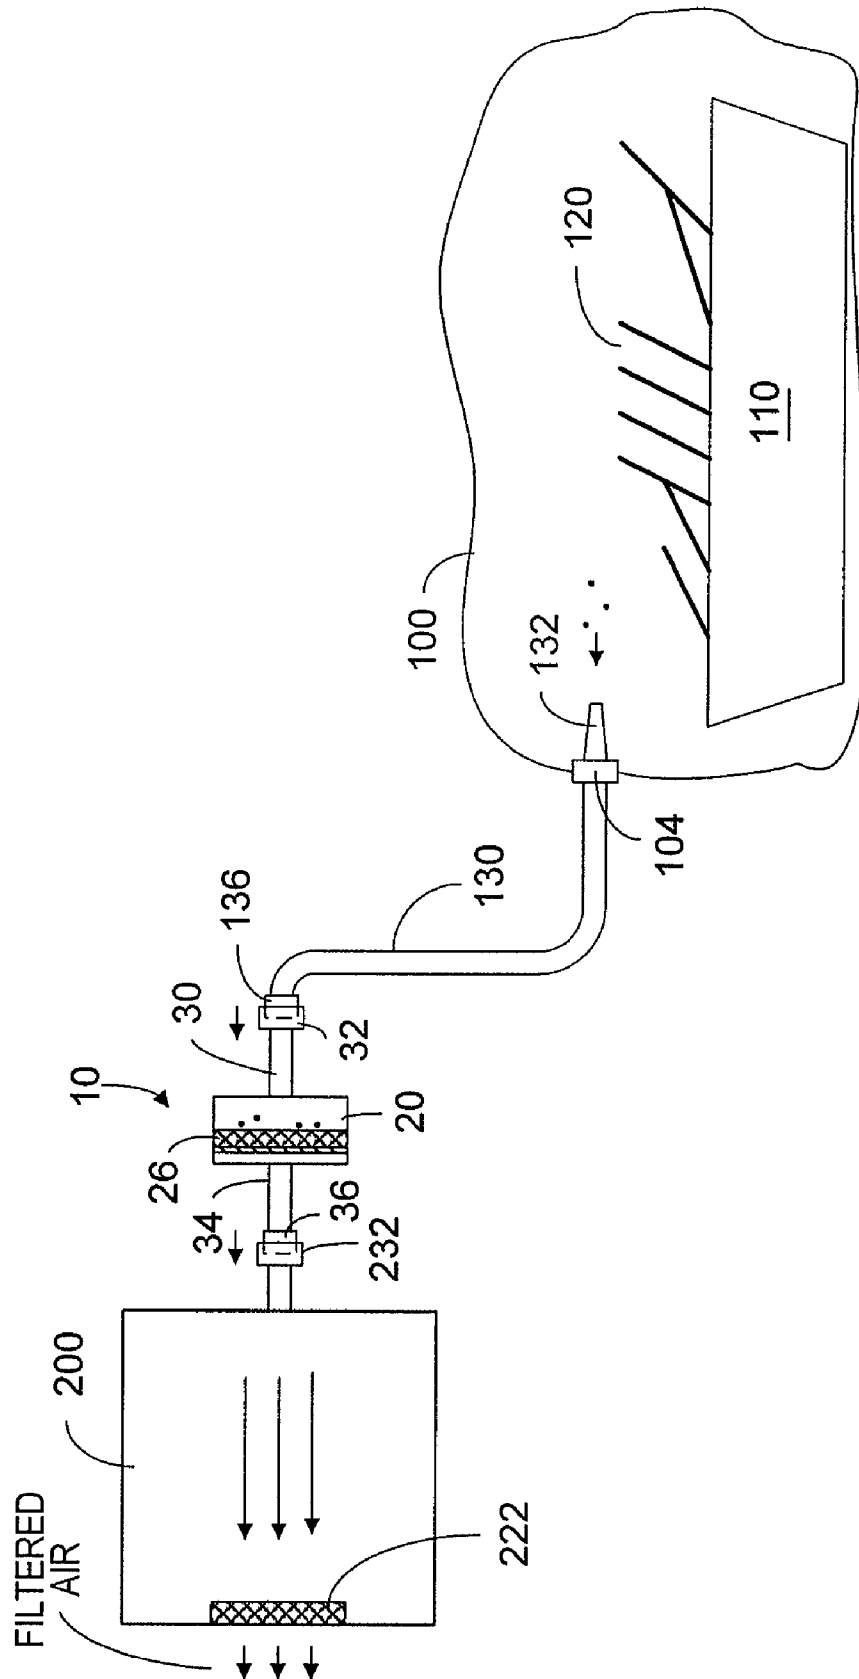
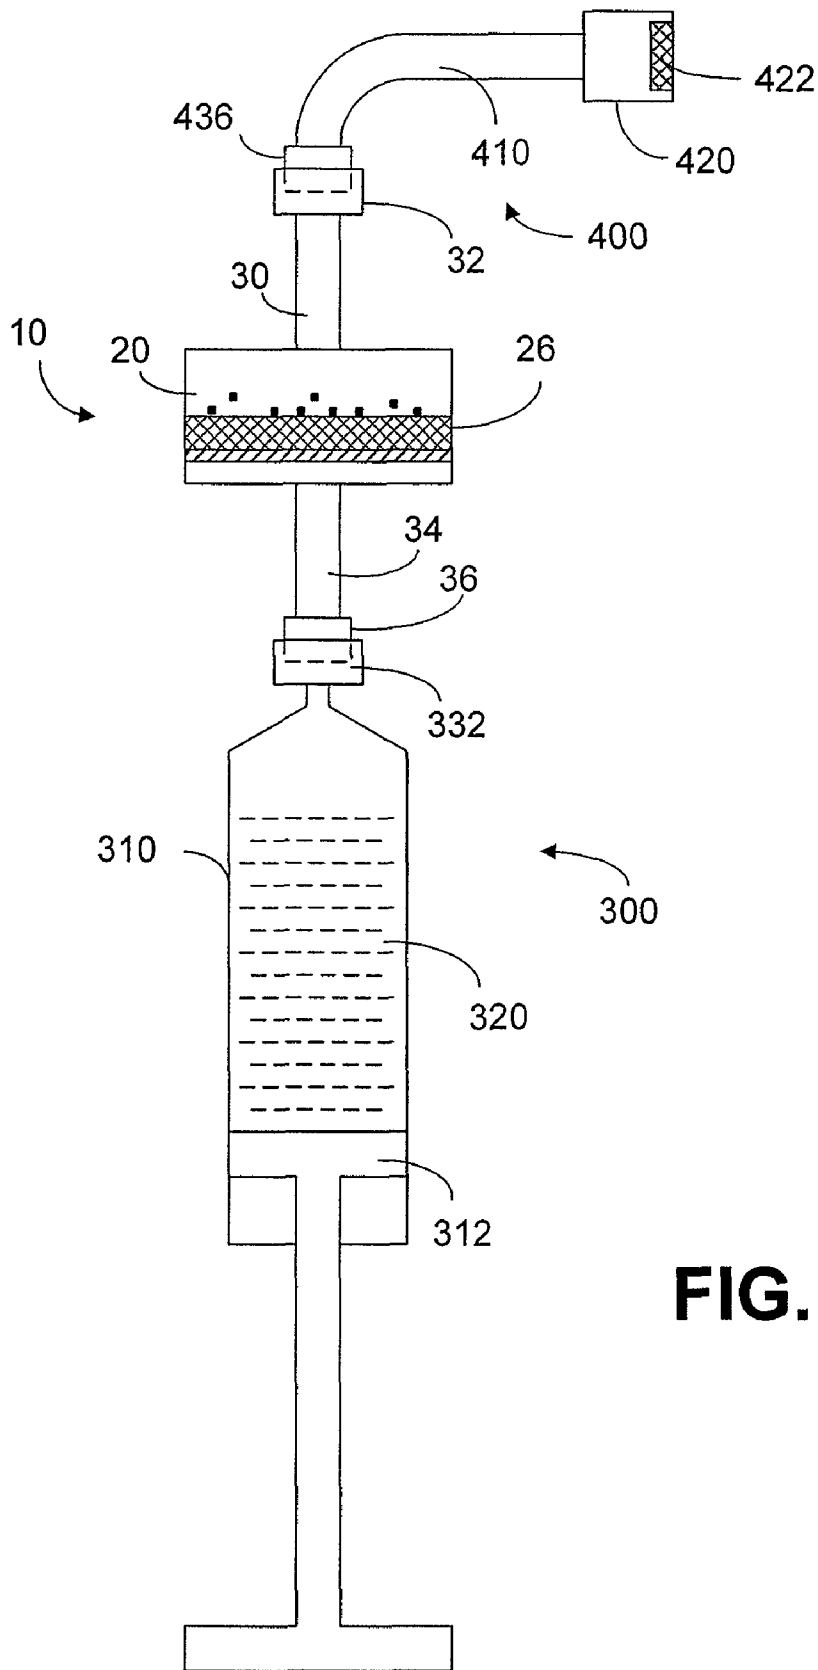
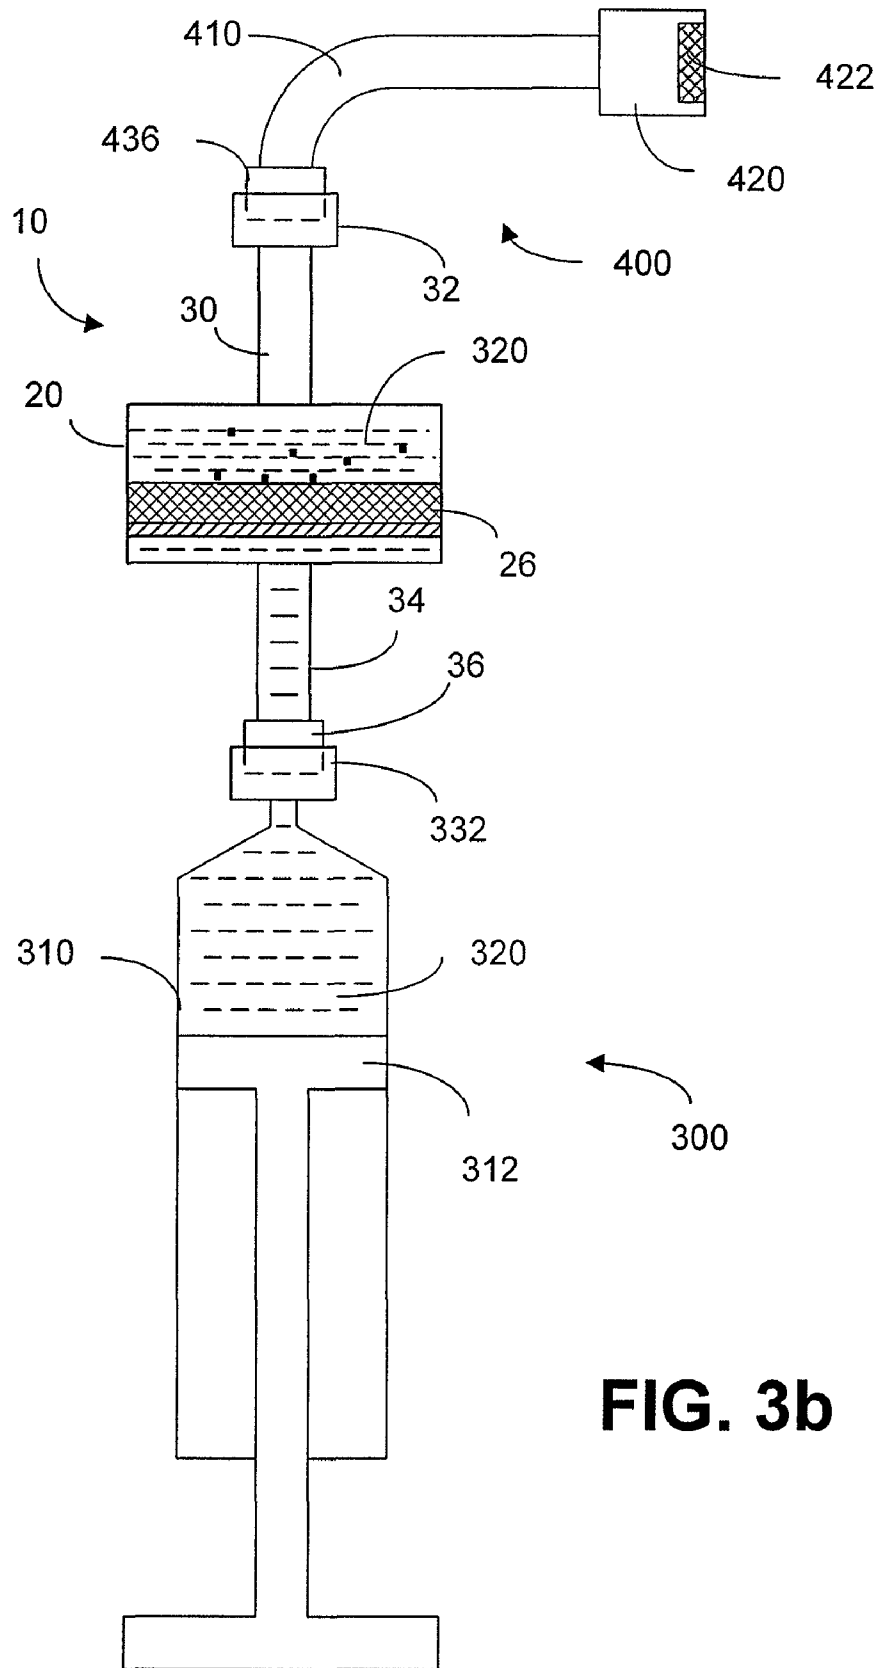


FIG. 2



**FIG. 3a**



**FIG. 3b**

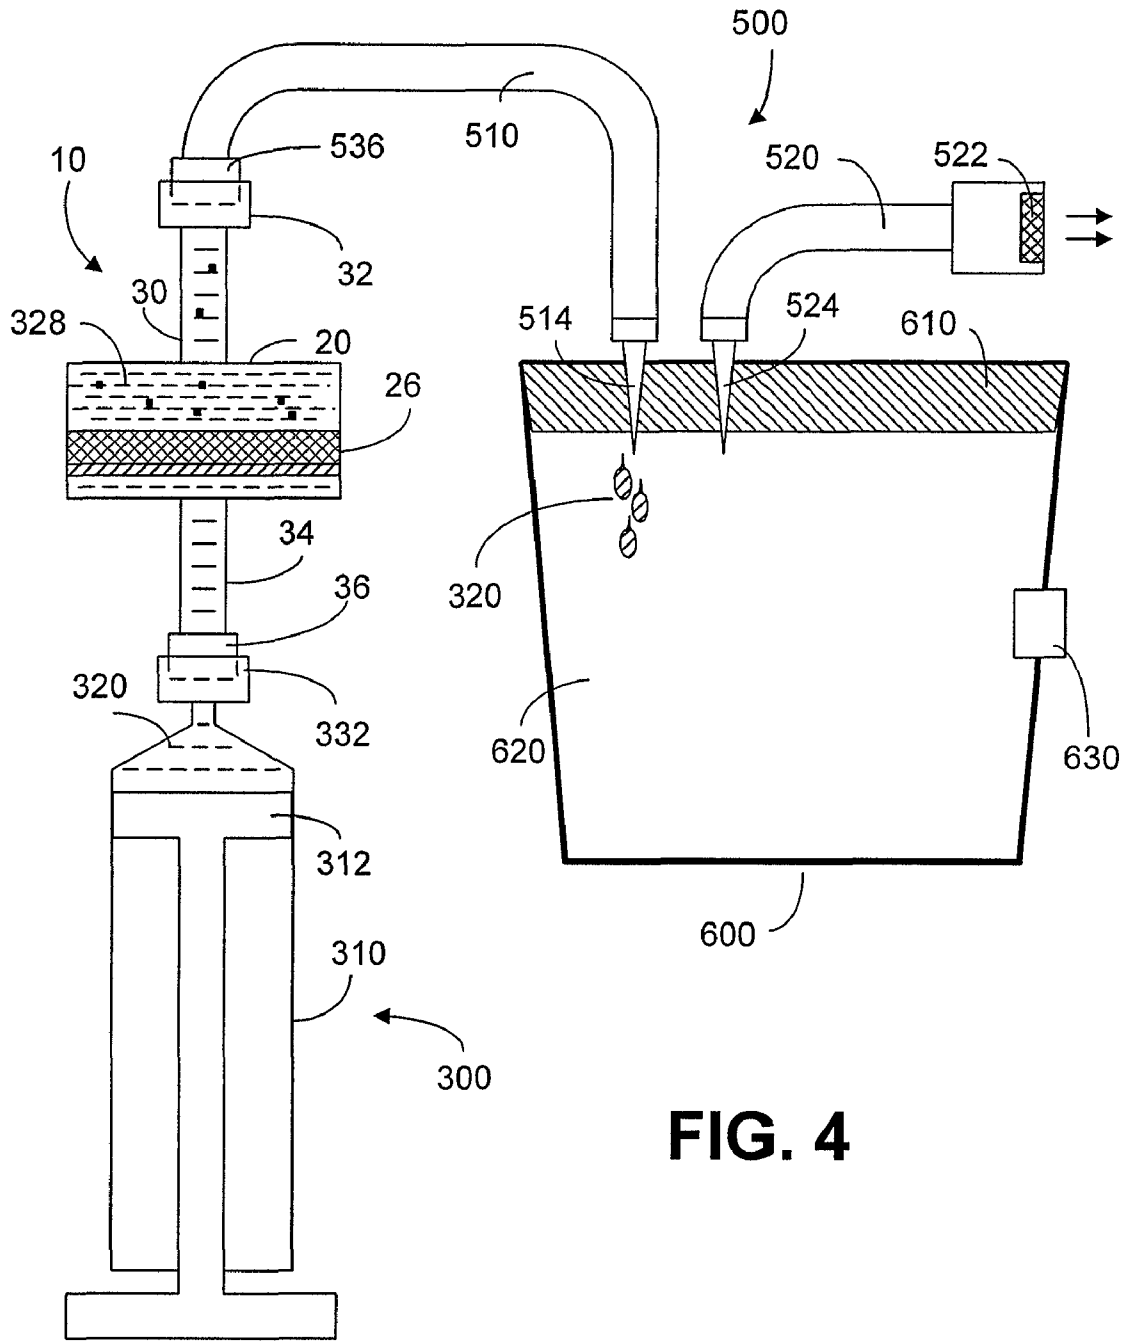


FIG. 4

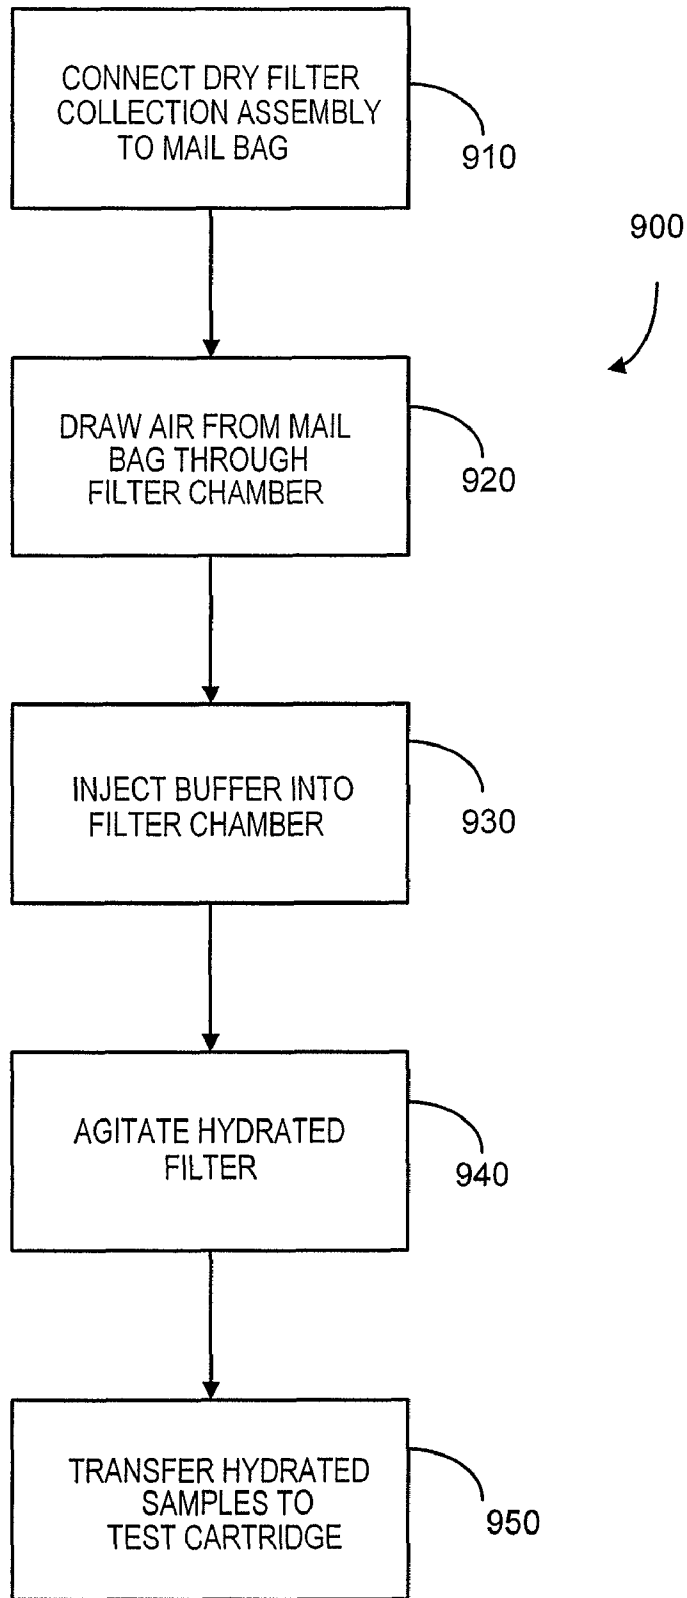


FIG. 5

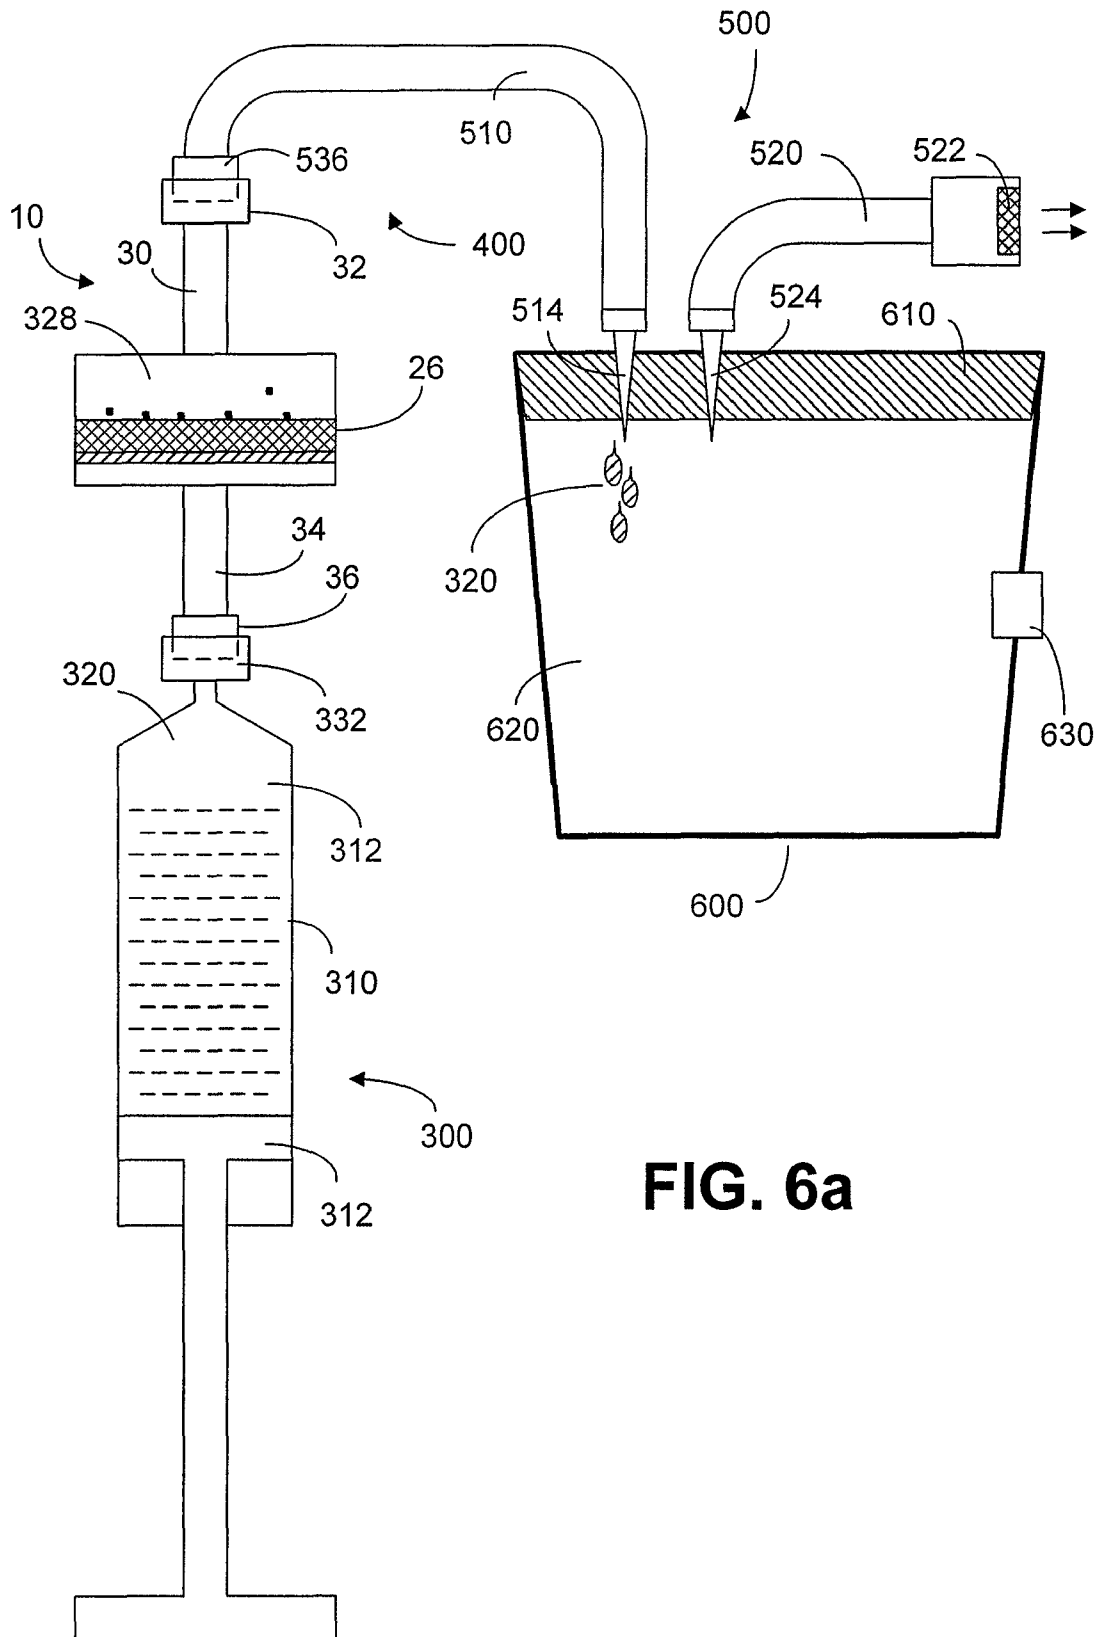


FIG. 6a



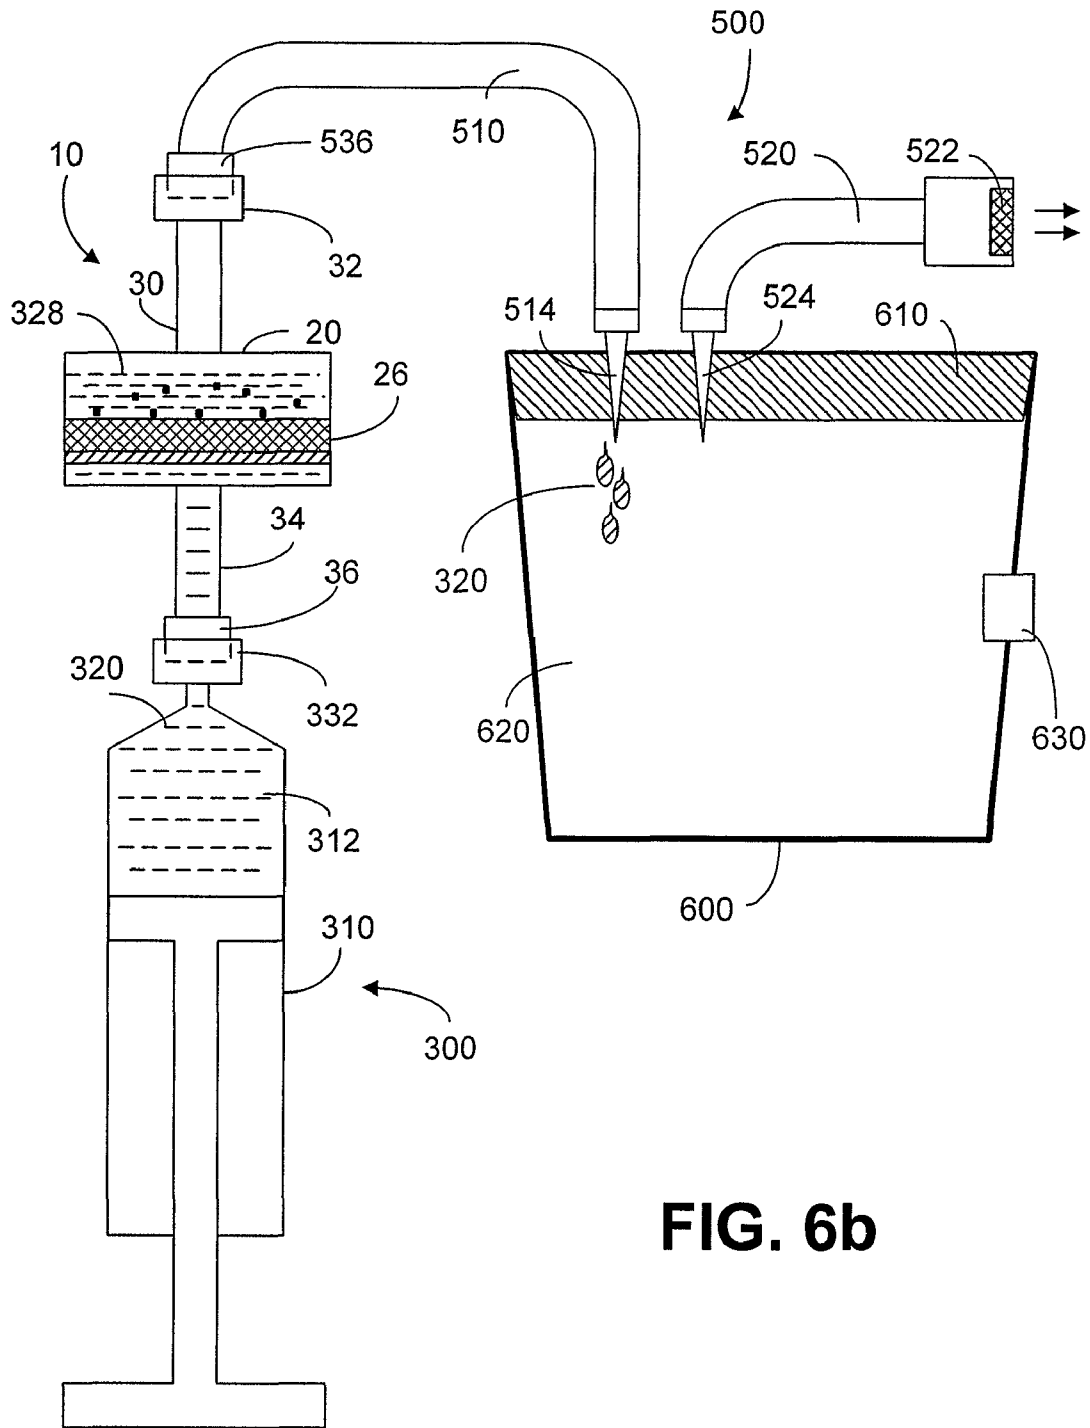


FIG. 6b

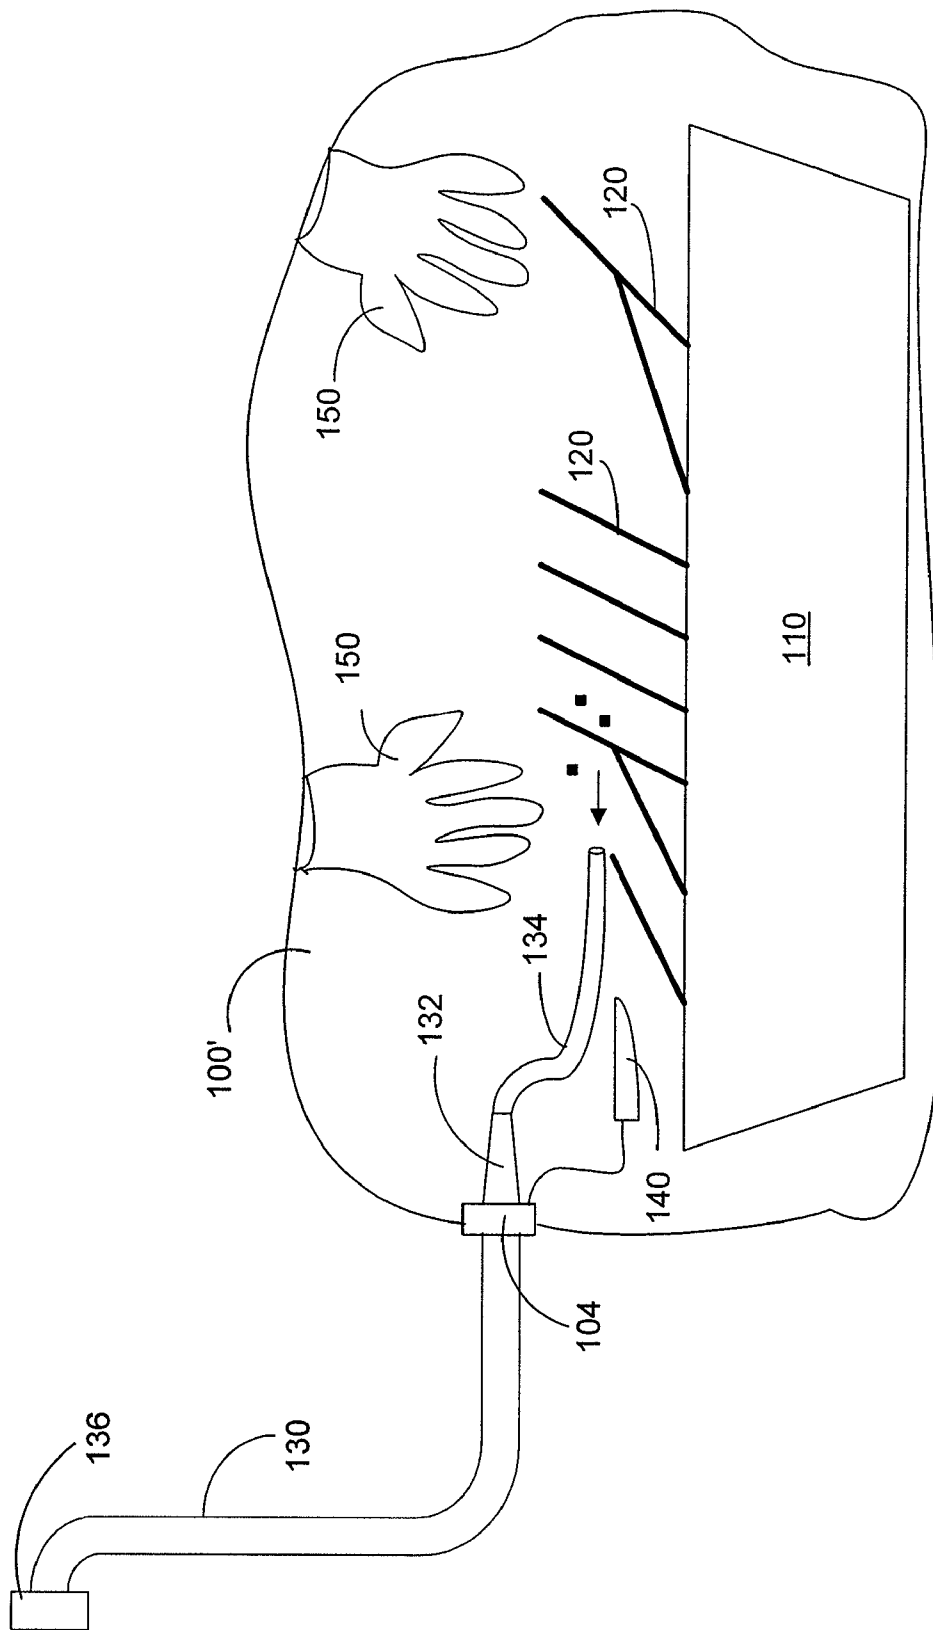


FIG. 7

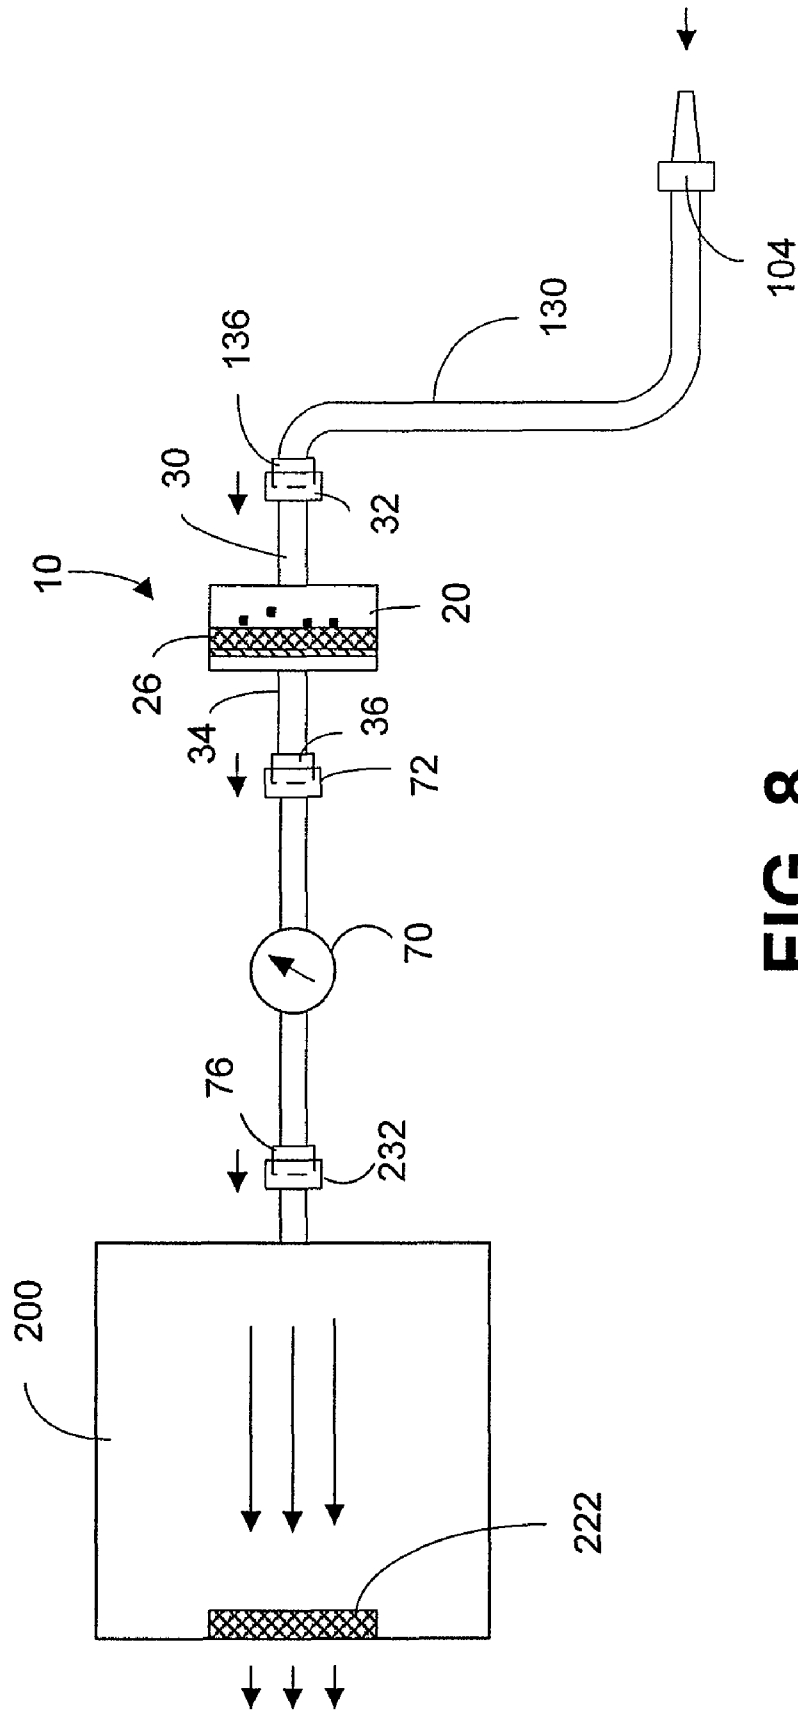


FIG. 8

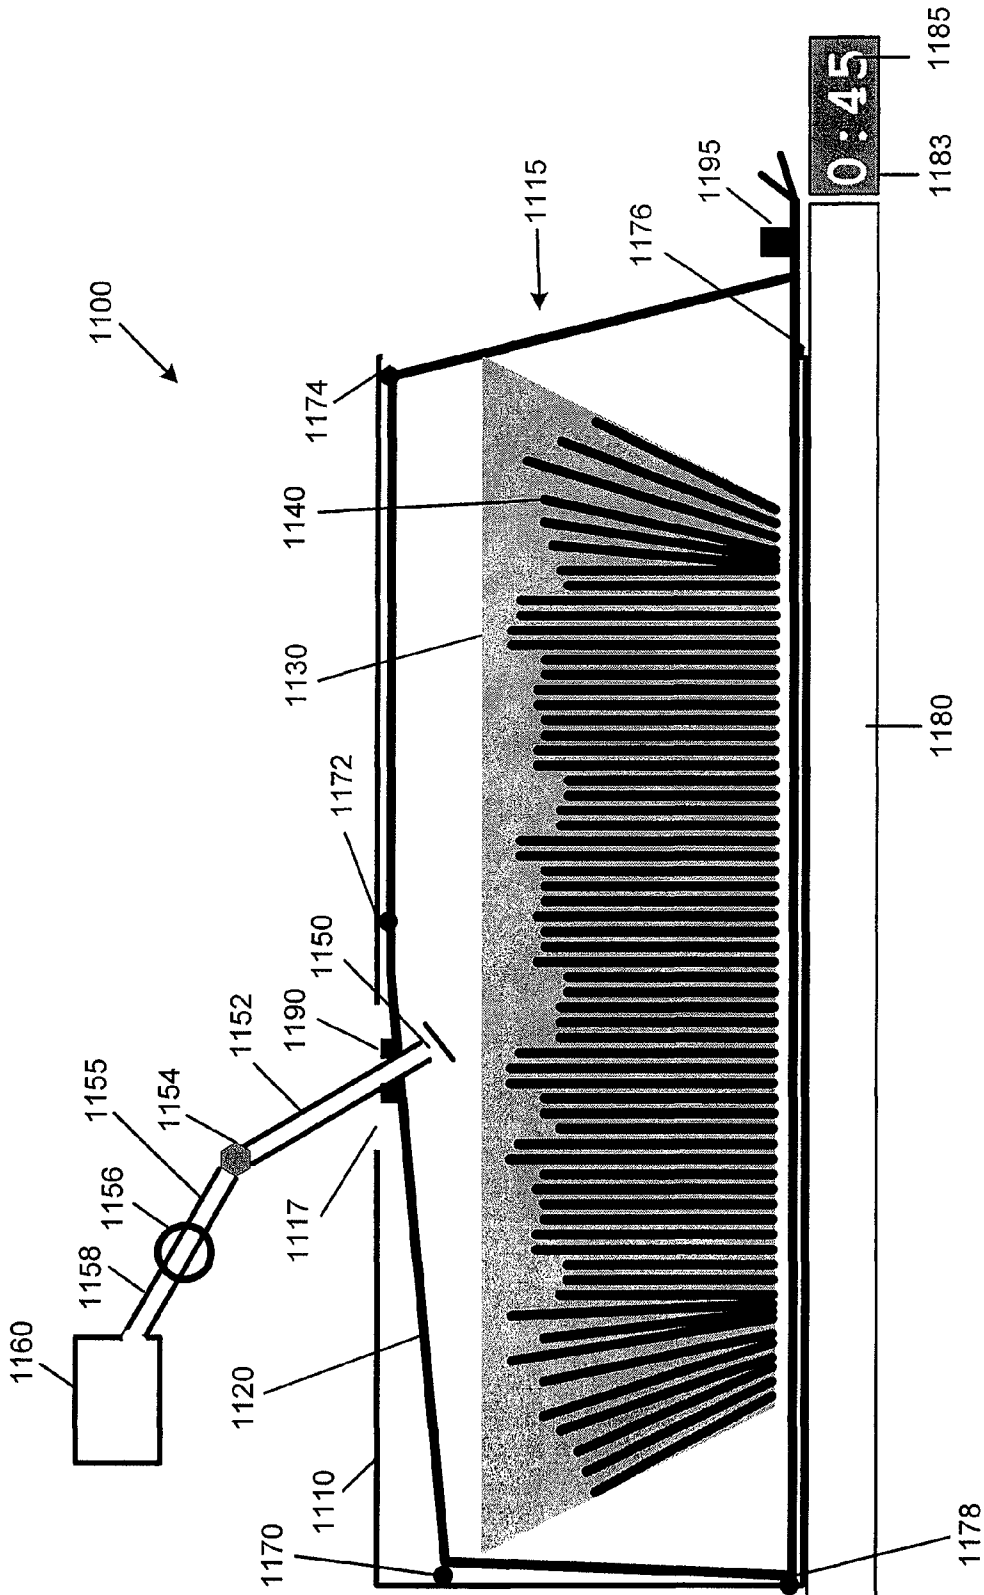


FIG. 9

## METHOD AND DEVICE FOR COLLECTING AND TRANSFERRING BIOHAZARD SAMPLES

### RELATED APPLICATIONS

The present application is a continuation-in-part of commonly owned U.S. patent application Ser. No. 10/741,264, filed Dec. 19, 2003, entitled "Method And Device For Collecting And Transferring Biohazard Samples" in the names of Douglas B. Quine, Ashwani Sharma, and John E. Massucci that is hereby incorporated by reference in its entirety. The present application is related to commonly owned, U.S. Pat. No. 7,060,927 B1, issued Jun. 13, 2006, entitled Method and System For Isolating And Testing Biological Contaminants In Mail Packages and commonly owned, U.S. Pat. No. 7,340,970 B2, issued Mar. 11, 2008, entitled Method And Device For Isolating, Collecting And Transferring Hazardous Samples both of which are hereby incorporated by reference in their entirety.

### FIELD OF THE INVENTION

The present invention relates generally to biohazard detection and, more particularly, to the transferring of a biohazard sample trapped in a filter to a detection system.

### BACKGROUND OF THE INVENTION

In late 2001, several United States postal offices and other buildings were contaminated with *Bacillus anthracis* spores (anthrax) along the eastern United States, resulting in anthrax infection and death among several individuals. This incident was quite costly, not only in terms of the health-related impact, but also in the required decontamination efforts. Cleanup following the anthrax contamination proved to be difficult, labor intensive, and expensive. As this threat still exists, there exists a need to detect biological contaminants within the postal packages or other containers.

Detection of biohazards in the mail for culture or polymerase chain reaction (PCR) analysis requires collection of a sample. Because biological contaminants such as anthrax can be easily carried in the air, aerosolization is an effective way to stir up a sample for collection using a dry filter. Ultimately, however, current biological test systems, such as the PCR test unit made by Cepheid (Sunnyvale, Calif.), require wet samples to detect the existence of certain biological contaminants including anthrax. For analysis, it is therefore necessary to hydrate the dry filter sample and transfer it to the analysis system. However, existing wet sample collectors are expensive and the collection efficiency is low.

Thus, it is advantageous and desirable to provide a method and device for collecting dry biological contaminants and hydrating the collected samples for transfer.

### SUMMARY OF THE INVENTION

The present invention provides a method and system for collecting particles that may be biological contaminants from the air in a mail container or the like. In the collection step, a dry filter collection assembly is connected to the mail container so as to allow air in the mail container to be drawn through a dry filter in the collection assembly. After this collection step, the filter collection assembly is disconnected from the mail container. A self-seal coupler, securely affixed to the collection assembly, is used to provide the connection between the collection assembly and the container, such that

when the collection assembly is connected to the container, the coupler is opened to allow air to pass through. But when the collection assembly is disconnected from the container. The coupler becomes self-sealed, thereby preventing the collected particles in the collection assembly from leaking out.

After the filter collection assembly is disconnected from the mail container, a syringe or the like is used to inject a certain amount of hydration solution into the collection assembly to hydrate the collected particles. An agitation process is used to suspend at least part of the collected particles in the hydration solution. The filter collection assembly is connected to a test cartridge and part of the hydration solution containing the collected particles is caused to move out of the collection assembly to the test cartridge.

The present invention will become apparent upon reading the description taken in conjunction with FIGS. 1 to 7.

### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a schematic representation illustrating a filter collection assembly having a filter for collecting small airborne particles.

FIG. 2 is a schematic representation illustrating the filter collection assembly being connected to a mail container for collecting airborne particles in the mail container.

FIG. 3a is a schematic representation illustrating the filter collection assembly being connected to a liquid providing device containing a hydration solution.

FIG. 3b is a schematic representation illustrating part of the hydration solution is injected into the filter collection assembly for hydrating the collected particles.

FIG. 4 is a schematic representation illustrating the liquid providing device is used to inject additional amount of hydration solution in order to move part of the hydration solution containing the collected particles into a test cartridge.

FIG. 5 is a flowchart illustrating the method of collecting particles and transferring the hydrated particles for testing, according to the present invention.

FIG. 6a is a schematic representation illustrating the liquid filter collection assembly being directly providing on a test cartridge.

FIG. 6b is a schematic representation illustrating part of the hydration solution is injected into the filter collection assembly for hydrating the collected particles.

FIG. 7 is a schematic representation illustrating a glove bag used as a mailbag.

FIG. 8 is a schematic representation illustrating an airflow gauge being used in conjunction with an air pump system.

FIG. 9 is a schematic representation illustrating an alternative system for collecting and transferring biohazard samples according to another illustrative embodiment of the present application.

### DETAILED DESCRIPTION OF THE INVENTION

The present invention uses a dry filter collection assembly to collect the biological contaminants from a sealed mailbag or container containing one or more mailpieces. The collected samples in the assembly are hydrated and then transferred to a test cartridge for testing. According to the preferred embodiment of the present invention, the collection assembly has two passageways to allow air or liquid to pass through. As shown in FIG. 1, the collection assembly 10 has a filter chamber 20 operatively connected to a first passageway 30 and a second passageway 34. The filter chamber 20 comprises a filter holder 24 to support an air filter 26. The pores on the filter 26 are about 0.8 microns in diameter. The first passageway 30 is

securely affixed to a first coupler **32**, which is self-sealed. This means that the passageway is substantially airtight when the first coupler **32** is not engaged with a matching coupler. The second passageway **34** is securely affixed to a second coupler **36**, which is also self-sealed. It is advantageous that the coupler **32** and the coupler **36** are different such that the collection assembly can only be connected to a certain device in a certain way. For example, one of the couplers **32**, **34** is a “male” connector while the other is a “female” connector. Alternatively, they are of different shapes or sizes. The filter chamber may optionally contain a plurality of beads **28**, as described later in conjunction with the agitation process. In the contaminant collection process, the first passageway **30** of the collection assembly **10** is operatively connected to a mailbag **100**, which contains a mail tray **110** having one or more mailpieces **120**. As shown in FIG. 2, the mailbag **100** has a tubing **130**. One end of the tubing **130** is securely affixed to a self-sealed coupler **136**. The other end of the tubing has an open inlet **132** to allow air to be drawn out from the mailbag **100** through the filter chamber **20** of the collection assembly **10**, when the coupler **136** is engaged with the coupler **32**. The open inlet **132** may be shaped like a “T” or have a number of orifices so that there are multiple sub-inlets to prevent blockage of air flow in the event that the end of the inlet touches the inner walls of the mailbag **100**. The second passageway **34** of the collection assembly **10** is operatively connected to an air pump system **200** so as to allow air to be drawn out from the filter chamber **20** through an air filter **222**, when the coupler **36** is engaged with a coupler **232** on the air pump system **200**. It should be noted that the pores on the filter **222** should be small enough to prevent biological contaminants from passing through. For example, the filter **222** is a HEPA filter. Prior to or during the collection process, it would be advantageous to disturb the mailpieces **120** so as to cause the contaminants contained within the mailpieces to be released outside, or to cause the contaminants attached on the mailpieces to be dislodged and aerosolized. For example, the mailpieces can be disturbed by shaking the tray or by dropping the tray from a height of one foot. Preferably, the mailbag **100** is made of an anti-static material so that the released or dislodged contaminants do not become attached to the interior of the mailbag **100**. When the coupler **136** and the coupler **32** are disconnected from each other, each of the couplers **136**, **32** becomes self sealed. Likewise, when the coupler **36** and the coupler **232** are disconnected from each other, each of the couplers **36** and **232** becomes self-sealed. Thus, when the collection assembly **10** is disconnected from the mailbag **100** and the air pump system **200**, the collection assembly **10** is sealed at both first and second passageways **30**, **34**. Thus, the collected contaminants in the filter chamber **20** are prevented from being released to the surroundings. Likewise, the coupler **136** is sealed, preventing the contaminants in the mailbag **100** from being released into the air. As for the air pump system **200**, only the coupler **232** becomes self-sealed. Air can still pass through the filter **222**. However, any unexpected contaminants collected inside the air pump system **200** are prevented from passing through the filter **222**.

In the hydration process, the collection assembly **10** that has been disconnected from the mailbag **100** and the air pump system **200** is connected to a liquid injection system **300**, as shown in FIG. 3a. The liquid injection system **300** has a liquid containing body **310** securely connected to a coupler **332**, which can be engaged with the second coupler **36** of the collection assembly **10**. For example, the liquid containing body **310** can be a syringe for injecting a desirable amount of hydration solution **320** backward into the filter chamber **20** through the second passageway **34** in order to flush the col-

lected particles out of the filter **26** and into fluid suspension. On the other end of the collection assembly **10**, the first passageway **30** is securely connected to a filter system **400** so as to allow the air inside the filter chamber **20** to be released when the hydration solution **320** is injected into the filter chamber **20**. The filter assembly **400** is made of a tubing **410** having a coupler **436** on one end and a filter holder **420** on the other end. The filter holder **420** is used to support a HEPA filter **422** or the like. The coupler **436** is also self-sealed, but it can be engaged with the first coupler **32** so as to allow the air in the collection assembly **10** to exit through the tubing **410** and then the filter **422**. Preferably, in the hydration process, the collection assembly **10** is only partially filled with the hydration solution **320** from the liquid containing body **310**, as shown in FIG. 3b. For example, while the syringe is filled with a hydration solution, the plunger **312** is only partially depressed. As such, the remaining hydration solution can be used later in the transfer stage. At this stage, it is desirable to agitate the collection system **10** to cause the contaminants retained by the filter **26** to mix with the hydration solution in the filter chamber **20**. Agitation can be carried out in many ways. For example, it is possible to place the edge of a vortex head in a vortex device in contact with the collection system **10** so as to allow the vortex head to shake the collection system **10** for 10 seconds, for example. Further, it may be desirable to preload or introduce a plurality of glass or plastic beads **28** into the filter chamber **20**, as shown in FIG. 1, so that these beads can help dislodge the contaminants from the filter **26** during agitation.

After agitation, the filter assembly **400** is removed from the collection assembly **10**. A transfer system **500** is used to transfer part of the hydration solution **320** in the filter chamber **20** to a test cartridge **600** and a protruding test chamber **630** for data capture, which contains the chemistry **620** for PCR analysis. Preferably, the test cartridge **600** comprises a septum cover **610** for sealing the cartridge. The septum **610** allows an injection needle to puncture through. But when the needle is pulled off the septum, the septum becomes self-sealed. It should be noted that, in this transfer stage, the contaminants within the collection assembly **10** are in contact with a liquid. Thus, aerosolization of the biological contaminants is substantially avoided. As shown in FIG. 4, the transfer system **500** comprises an injection needle **514** connected to one end of a tubing **510**, and a coupler **536** is connected to the other end. The transfer system **500** also comprises an air-venting needle **524** connected to one end of another tubing **520**, and an air filter **522** connected to the other end. After the injection needle **514** and the air-venting needle **524** are adequately inserted into the test cartridge **600** through the septum cover **610**, more hydration solution is injected into the collecting assembly **10** in order to push part of the hydration solution **320** inside the filter chamber **20** into the test cartridge **600**. The displaced air is filtered by filter **522** to prevent release of any contaminants into the room. Before removing the test cartridge **600** from the transfer **500** so that the test cartridge can be placed in a test device for contaminant detection, it is preferable to withdraw the remaining liquid in the needle **514**, the tubing **510** and the coupler **536** by backing off the syringe **300**.

It should be noted that the test cartridge **600** for PCR analysis contains a plurality of separate chemical chambers for carrying out PCR processes. Thus, the injection needle **514** must be inserted through the septum cover **610** in the correct position so that the hydration solution is injected into the correct chamber. It is possible that the transfer system **500** has a keyed shape that fits the test cartridge only in a certain way so as to ensure the needle **514** punctures the septum in the

5

correction position. Moreover, if the amount of hydration solution injected into the cartridge **600** is small, it may not be necessary to provide the air-venting needle **524** for air venting as long as the injection does not result in pressurizing the system. In an alternative embodiment, the transfer system **500** is also to preload the necessary chemical solutions into the test cartridge **600**. One or more additional needles may be positioned on the transfer system **500** to introduce the chemical solutions into the chemical reaction chambers or to puncture the sealed bladders within these chemical reaction chambers for releasing the chemical solutions preloaded in the bladders.

In sum, the method of collecting contaminants from a container such as mailbag and transferring the collected contaminants to a test cartridge, according to the present invention, is illustrated in the flowchart **900** in FIG. **5**. As shown, a dry filter collection assembly **10** is connected to a mailbag **100** at step **910**. The dry filter collection assembly **10** is also connected to an air pump system **200** so as to allow air in the mailbag to be drawn through the filter collection assembly **10** at step **920**. After the filter collection assembly **10** is disconnected from the mailbag, a hydration solution is injected into the filter collection assembly at step **930**. The filter collection assembly **10** is agitated, at step **940**, in order to suspend at least part of the collected contaminants in the hydration solution. Finally, more liquid is injected into the filter collection assembly, at step **950**, in order to push some of the hydration solution containing the contaminants into the test cartridge.

It should be noted that many components in the collection/transferring device, according to the present invention, are available as off-the-shelf products. For example, the dry filter collection assembly **10** can be modified from a filter cassette (Omega A0037503) supplied by BGI (Waltham, Mass.). The filter **26** is an Omega M083700P filter supplied by BGI. The filter is 37 mm MCE (mixed cellulose ester) 0.8 micron filter with a backing pad. This filter has been shown to capture substantially all anthrax spores. The coupler **32** is a self-seal male connector and the coupler **36** is a self seal female connector (62860-288 connector pair) made by VWR International (West Chester, Pa.) or PLCD170412 and mate made by Colder Products Corp (St. Paul, Minn.). The mailbag **100** is an aegis pink 36"×42"×0.004 anti-static poly bag with amines, Part No. 3508 supplied by Marathon Plastics, Inc. (Shelton, Conn.). The filter **222** is HEPA filter made by Whatman, Inc. (Clifton, N.J.). The test cartridge **600** is a 4 plex anthrax test cartridge made by Cepheid (Sunnyvale, Calif.) for use in a GeneXpert PCR 4-channel test system made by Cepheid. However, these products can be substituted by equivalents.

It should be noted that when the hydration solution is injected into the filter collection assembly at step **930**, it is desirable that the amount of injected hydration solution is predetermined such that the filter chamber **20** is only partially filled. As such, the hydration solution in the filter chamber **20** can be easily agitated with a vortex device or the like. Accordingly, it is desirable to have a marking, indicative of the predetermined amount, provided on the syringe so that the person who depresses the plunger knows when to stop depressing the plunger. It is possible that a stopping device is used to limit the depressing of the plunger when needed. It is also possible to use two different syringes to provide a liquid to the filter chamber: one in the hydrating step and the other in the transferring step. It is also possible to move part of the hydration solution containing the particles out of the filter chamber to the test cartridge by injecting air into the filter chamber through the second passageway **34**.

6

In a different embodiment, the transfer system **500** is securely attached to the test cartridge **600** as an integral part thereof. It is also possible that before the liquid injection system **300** is used to inject the hydration solution into the filter chamber **20**, the first passageway **30** is directly connected to the transfer system **500** with the coupler **32** engaged with the coupler **536**, as shown in FIG. **6a**. The collection assembly **10** is then partially filled with the hydration solution **320**, as shown in FIG. **6b**. After the filter chamber **20** is agitated to further dislodge the collected particles from the filter **26**, additional solution is injected into the collection assembly in order to push part of the hydration solution **320** inside the filter chamber **20** into the test cartridge **600**, as shown in FIG. **4**. The hydration solution can be distilled water or a buffer solution.

In another embodiment, the collection assembly **10** and the transfer system are integrated with the test cartridge **600** as a single functional unit, thereby eliminating the need for many of the self-sealing couplers. While the Cepheid GeneXpert System is designed for use with stand alone test cartridges, a low profile transfer device **500** could be attached on top of the test cartridge **600** and left in place as it is placed into the analysis device. Thin tubes and structural connections could be aligned to exit through the gaps around the GeneXpert door (or the door could be removed/modified) so that the collection, transfer, and test device could remain as a single sealed unit even during sample analysis.

It is possible that the mailbag **100'** is a glove bag having a pair of gloves **150** so as to allow a person to access the mailpieces **120** inside the bag **100'** through the gloves, as shown in FIG. **7**. A flexible tube **134** is extended from the inlet **132** so that it can be inserted into each of the mailpieces **120** for directly collecting particles in individual mailpieces. It is also possible to provide a cutter **140** inside the mailbag **100'** to make a small slit cut on the mailpieces so as to allow the flexible tube **134** to be inserted into the slit cut.

It is advantageous to install a flow gauge in the filter collection assembly to monitor the air flow. For example, an air flow gauge **70** having couplers **72** and **76** is installed between the air pump system **200** and the collection assembly **10**, as shown in FIG. **8**. The air flow gauge **70** could be a valuable element in that it provides a confirmation that air is being successfully sampled from the mailbag **100**. The gauge **70** also provides objective demonstration of the air flow rate (6 liters per minute, for example). If the air flow is blocked, this may indicate that the tubing is kinked, the mailbag has been completely evacuated, or the self-sealing couplers are not properly engaged. For example, flow gauge 20 SCFH with tube fittings from King Instrument Company (Garden Grove, Calif.) can be used for such purposes. The air flow gauge may provide audio indication that the flow is not normal.

Referring to FIG. **9**, a schematic representation illustrating an alternative system **1100** for collecting and transferring biohazard samples according to another illustrative embodiment of the present application is shown. The system **1100** is illustrated in a side view cross section. A rectangular box **1110** or other suitably shaped box to contain trays **1130** is constructed of a suitable material such as a clear Plexiglas closed on 5 sides and open on one side, e.g. the right side **1115** (or with a door that may open). The opening **1115** (or door) provides the opening to the so called garage (the box **1110**) in which the trays of mail **1130** will be parked for sampling in an anti-static container **1120** such as an anti-static bag. Here, the garage is lined with a replaceable plastic anti-static bag **1120**. The inside of the plastic bag should contain no new materials beyond those included in any initial spore test. Accordingly, it may be advantageous to have the bag inside the rigid struc-

ture, rather than having the rigid structure inside the bag. It is preferable that aerosolized spores not be attracted to or stick to the garage material. Therefore, the bag 1120 is attached to the inside of the box by fasteners such as glue, or removable fasteners such as clamps or VELCRO hook and eye fasteners 1170, 1172, 1174, 1176, 1178 to keep the bag expanded to the rough dimensions of the rigid garage 1110. Such bags have been tested as part of a Biohazard Isolation and Screening system (BISS) and are now known to be capable of use for the containment and collection of biohazard spores. A sample collection tube 1152 with a "T" shaped end 1150 is inserted into the top of the bag and sealed with a tie wrap or clamp 1190. The branched air inlet 1150 helps ensure that it cannot be blocked if the end makes contact with the plastic bag material. The sample collection tube 1152 passes out of the garage 1110 through a hole 1117, to the pharmaceutical self sealing connector 1154. It continues through tube 1155 to the sample collection filter 1156 and then through an additional tube 1158 to the BISS handheld vacuum unit 1160. The antistatic bag 1120 and the sample collection components 1150, 1152, 1154, 1155, 1156, 1158, and 1160 are described more fully above and in the related incorporated applications. The present illustrative embodiment uses many of the features and materials described as effective in the related applications even though the external appearance and operational processes have been modified to reflect the different operating environment for this configuration.

In operation, a mail tray 1130 containing a plurality of mail pieces 1140 is placed inside the anti-static plastic bag 1120. The plastic bag 1120 is then sealed shut with a tie wrap, Velcro strap, or preferably a hinging bar 1195 which folds down to seal the bag shut across the entire length of the opening. Such a closure device 1195 can be operated quickly with one hand. Alternatively, a rubber lining on the edge against the plastic bag would ensure that a tight form fit could be maintained to make a good seal. The entire garage 1110 is rigidly attached to a jogger platform 1180 which allows the garage, bag, mail tray, and mail pieces to be agitated and thereby aerosolize spores within the mail for collection on the BISS filter 1154 when air is drawn by the handheld vacuum 1160. One useful protocol provides for the mail to be agitated for 45 seconds after which the clamp 1195 may be released. The mail tray 1130 containing mail 1140 may then be removed through the opening 1115 and another tray inserted into the station to repeat the process. Use of two such jogger/collection stations would allow the pharmaceutical connector 1154 to be disconnected from the first station and connected to a tray loaded into the second station for collection while the first station was being reloaded. In this manner, system throughput can be maintained with a tray being processed every 45 seconds (the sample collection time). As soon as one tray collection is complete, the tube is switched to the other work station and collection commences there with barely a second of delay. The operator then has nearly 45 seconds to exchange mail trays in the first station. This task would be expected to require only 5 or 10 seconds, thereby allowing an operator sufficient time for staging trays, delivering them to the adjacent work flow processes, or data recording while the pump runs continuously.

A smooth work surface 1183—possibly with rollers—at the same elevation as the "garage" floor would allow the trays to be slid into the ergonomic biohazard sampling station without the need for any additional lifting. A resettable digital timer 1185 allows the operator to time the samples and observe how much time remains on the current sampling cycle. The biohazard work station 1100 could be easily operated by a single employee. At 45 seconds per tray, the

employee would be able to process approximately 80 trays per hour. Such efficiency compares very favorably with prior testing processes that often require considerably more hardware and an additional operator. This embodiment and alternatives described and referred to may be utilized with any of the embodiments described and referred to in the incorporated related applications as practical.

It should be also noted that the filter collection system, according to the present invention, allows for the creation of a sample volume greater than that required for a single test run so that the same sample can be used for re-testing if needed.

Thus, although the invention has been described with respect to a preferred embodiment thereof, it will be understood by those skilled in the art that the foregoing and various other changes, omissions and deviations in the form and detail thereof may be made without departing from the scope of this invention.

What is claimed is:

1. A method for collecting particles that may be contaminants from the air in a container, comprising:
  - providing a collection assembly having a filter chamber; operatively connecting the collection assembly to the container;
  - agitating the container;
  - while agitating the container, drawing at least part of the air from the container through the filter chamber of the collection assembly so as to collect in the filter chamber the particles in the air drawn from the container; and
  - mixing in the filter chamber at least part of the collected particles with a liquid.
2. The method of claim 1, wherein the collected particles are transferred to a test cartridge for testing, said method further comprising:
  - operatively connecting the collection assembly to the test cartridge; and
  - moving at least part of the liquid in the filter chamber to the test cartridge.
3. The method of claim 2, further comprising agitating the liquid in the filter chamber prior to said moving so as to increase the part of the collected particles mixed with the liquid.
4. The method of claim 1, further comprising injecting the liquid into the filter chamber after said drawing and prior to said mixing.
5. The method of claim 4, wherein the liquid injected into the filter chamber is substantially retained in the filter chamber in said mixing.
6. The method of claim 2, wherein the collection assembly has a first passageway and a second passageway separately extended from the filter chamber, and wherein the first passageway is operatively connected to the container for operatively connecting the collection assembly to the container, said method further comprising operatively connecting the second passageway to an air drawing system for drawing said part of the air from the container through the first passageway, the filter chamber and then the second passageway.
7. The method of claim 6, further comprising disconnecting the second passageway from the air drawing system after said drawing, and operatively connecting the second passageway to a liquid providing device so as to allow the liquid providing device to provide the liquid in the filter chamber through the second passageway prior to said mixing.



9

8. The method of claim 7, further comprising disconnecting the first passageway from the container after said drawing; and  
 operatively connecting the first passageway to the test cartridge for operatively connecting the collection assembly to the test cartridge. 5

9. The method of claim 8, further comprising further providing a further amount of liquid to the second passageway after said mixing and operatively connecting the first passageway to the test cartridge so as to move said at least part of the liquid in the filter chamber to the test cartridge. 10

10. The method of claim 7, wherein the amount of the liquid provided to the filter chamber by the liquid providing device is predetermined to suit the size of the filter chamber and the second passageway. 15

11. The method of claim 1, further comprising disturbing the container so as to stir up the particles in the container into the air in the container. 20

12. The method of claim 1, wherein the container containing one or more mailpieces, said method further comprising disturbing said one or more mailpieces so as to stir up the particles associated with said one or more mailpieces. 25

13. A method for collecting particles that may be contaminants from the air in an antistatic lined resealable container, comprising:  
 providing a collection assembly having a filter chamber; operatively connecting the collection assembly to the container; 30  
 agitating the container;  
 while agitating the container, drawing at least part of the air from the container through the filter chamber of the collection assembly so as to collect in the filter chamber the particles in the air drawn from the container as a sample; and 35  
 subsequently transferring the sample to an analysis device.

14. The method of claim 13, wherein, 40  
 the container is resealed with a door.

10

15. The method of claim 13, wherein, the container is resealed with a clamping device around the antistatic lining.

16. The method of claim 13, wherein, the container is resealed with a reusable fastener.

17. The method of claim 13, wherein, the container is resealed with a tie wrap.

18. A method for collecting particles that may be contaminants from the air in a container, comprising:  
 providing a collection assembly having a filter chamber; operatively connecting the collection assembly to the container;  
 drawing at least part of the air from the container through the filter chamber of the collection assembly so as to collect in the filter chamber the particles in the air drawn from the container; and  
 mixing in the filter chamber at least part of the collected particles with a liquid, wherein, the collected particles are transferred to a test cartridge for testing, said method further comprising:  
 operatively connecting the collection assembly to the test cartridge;  
 moving at least part of the liquid in the filter chamber to the test cartridge;  
 agitating the liquid in the filter chamber prior to said moving so as to increase the part of the collected particles mixed with the liquid; and  
 providing beads in the filter chambers for agitating the liquid in the filter chamber.

19. The method of claim 1, further comprising:  
 before mixing in the filter chamber at least part of the collected particles with a liquid,  
 operatively connecting the collection assembly to a second container; and  
 drawing at least part of the air from the second container through the filter chamber of the collection assembly so as to collect in the filter chamber the particles in the air drawn from the second container.

20. The method of claim 19, further comprising:  
 while drawing at least part of the air from the second container, agitating the second container.

\* \* \* \* \*